

MD SalivaScreen

DRUG TEST

PRODUCT FEATURES:

- Sponge saturation indicator
- Non-negative results in 5 minutes
- Alcohol or EtG Test also available
- Individually sealed saliva collectors
- Screen up to 14 drugs per device
- Read drug test results in 5-10 minutes and alcohol test in 2-5 minutes
- Non-invasive and decent collection
- Minimal chances of adulteration and contamination
- Avoids cross gender observation
- More sensitive parent THC detection



MD SalivaScreen Drug Test configuration:

Amphetamine	(AMP)	Marijuana	(THC)
Barbiturates	(BAR)	Fentanyl	(FEN)
Buprenorphine	(BUP)	Methadone	(MTD)
Benzodiazepine	(BZO)	Methamphetamine	(MET)
Cocaine	(COC)	Opiates	(OPI)
Ecstasy	(MDMA)	Oxycodone	(OXY)
Alcohol	(ETG)	Phencyclidine	(PCP)



Instructions

Please read first

IMPORTANT: Donors should not place anything (including food, drink, gum, or tobacco products) in their mouth for at least 10 minutes prior to the procedure. Do not bite, suck, or chew on the sponge. Refrain from talking while collection swab is in the mouth.




Follow these instructions for the best results with this innovative screening device, which includes market-leading drug cutoffs and the first-ever sponge saturation indicator.

STEP 1

The purpose of Step 1 is to saturate the sponge with saliva. With collection swab (B), have donor sweep the inside of mouth (cheek, gum, tongue) several times, then hold swab in closed mouth until instructed to remove it. Donor may remove swab from mouth when color appears in the indicator window.

Note: If at 7 minutes, color on saturation indicator has not appeared in indicator window, proceed with test (Step 2).

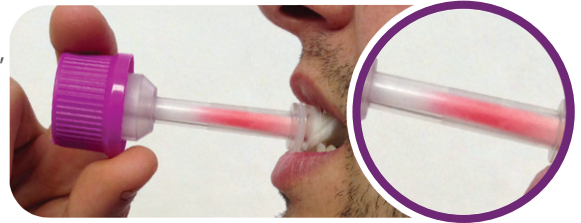


STEP 2

Remove collection swab from mouth and insert sponge first into screening device (A), pushing until locking flange locks in place in the bottom of device. Once locked in place the device airtight, tamper evident, and ready to dispose of after use or send to lab for confirmation (on presumptive positive result). Ensure that specimen is contacting all test strips. If not, rotate the device side to side/front to back to disperse the specimen within the chamber.


With specimen dispersed, set device upright on flat surface. Keep upright while test is running.



Screening Device

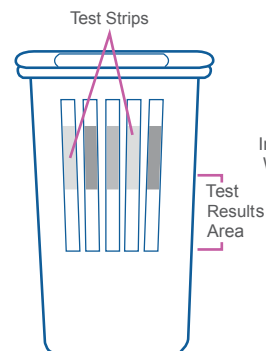

Collection Swab

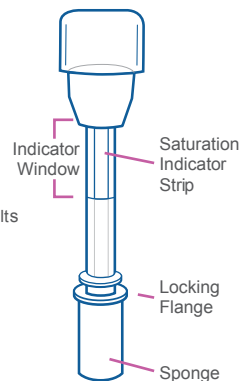



STEP 3

Read negative results as soon as two lines appear on any test strip, often within 2 minutes. Any indication of a line in the test region (T) should be considered a line, and therefore a negative result. Read presumptive results at 10 minutes.

Note: The THC (marijuana) strip has improved sensitivity, which may show a less intense color band in the test region (T). This is an expected and normal response.

If the device includes alcohol, read the alcohol strip at 2 minutes. Compare the color of the reaction pad with the color chart provided to determine the relative blood alcohol level. No color change indicates a negative result.

Interpret Results



EXAMPLE: Presumptive positive for cocaine (COC)

Saliva Alcohol Color Chart

Alcohol strips must be read in 2 minutes as pad color may change.

